

Nombre del Instrumento: Calibrador Vernier Num.Serie: 8000160 Marca: Mitutoyo
 Alcance: 150 mm Modelo: 501-100 Resolución: 0.01


RESULTADOS DEL ESTUDIO

Val.Ref.1: 2 Val.Ref.2: 4 Val.Ref.3: 6 Val.Ref.4: 8 Val.Ref.5: 10

Datos para Estudio Linealidad

Med.Val. Ref.1.	Med.Val. Ref.2.	Med.Val. Ref.3.	Med.Val. Ref.4.	Med.Val. Ref.5.
2.7	5.1	5.8	7.6	9.1
2.5	3.9	5.7	7.7	9.3
2.4	4.2	5.9	7.8	9.5
2.5	5	5.9	7.7	9.3
2.7	3.8	6	7.8	9.4
2.3	3.9	6.1	7.8	9.5
2.5	3.9	6	7.8	9.5
2.5	3.9	6.1	7.7	9.5
2.4	3.9	6.4	7.8	9.6
2.4	4	6.3	7.5	9.2
2.6	4.1	6	7.6	9.3
2.6	3.8	6.1	7.7	9.4

Gráfica Estudio Linealidad

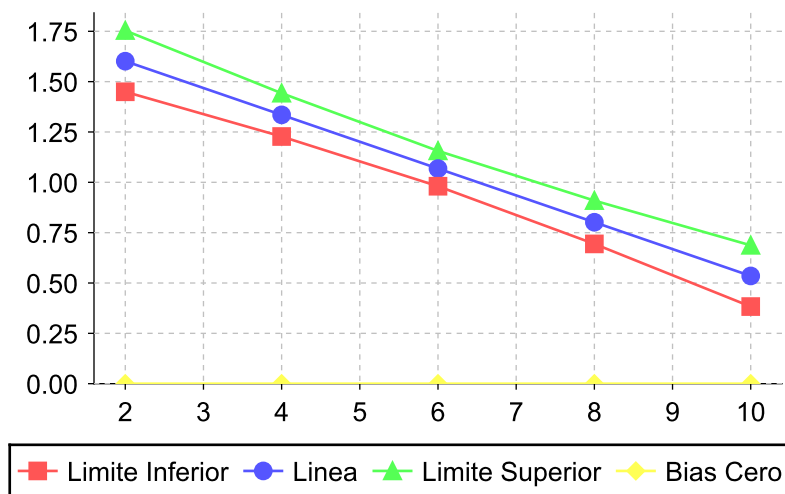

ANÁLISIS DE RESULTADOS

Val.Ref.	X0-Xbar	(X0-Xbar) ²	Relación	Suma	SQRT	CBV	Linea	Lim.Inf.	Lim.Sup.	Bias Cero
2.0	-4.0	16.0	0.03333333	0.05	0.223606797	0.152034075	1.6016666666	1.449632591	1.753700742	0.0
4.0	-2.0	4.0	0.00833333	0.025	0.158113883	0.107504325	1.3350000000	1.227495674	1.442504325	0.0
6.0	0.0	0.0	0.0	0.0166666	0.129099444	0.087776914	1.0683333333	0.980556418	1.156110247	0.0
8.0	2.0	4.0	0.00833333	0.025	0.158113883	0.107504325	0.8016666666	0.694162340	0.909170992	0.0
10.0	4.0	16.0	0.03333333	0.05	0.223606797	0.152034075	0.5350000000	0.382965924	0.687034075	0.0